



Ventia – EastLink Tunnel

Ventilation Stack Air Quality Monitoring Validated Data Report

01 October 2025 to 31 December 2025

Ref: DR. Q42025.ETL

Issue Date: 21/01/2026

Report prepared by: Tim Allfrey

Document Control

Revision	Date	Details	Prepared By	Approved By
0	21/01/2026	Original	TA	BN

Distribution

Format	Recipient	Details
PDF	George Vasiliadis	Gvasiliadis@connecteast.com.au
PDF	Robbie Kristenson	kristenson@connecteast.com.au

Prepared by

Tim Allfrey
 21 January 2026

Approved by

Bruno Nourdine
 21 January 2026

Norditech Accreditations

We operate a fully compliant NATA-approved lab, and our engineers are factory-trained in the repair and maintenance of most types of gas analysers on the market, including circuit board level repairs. Our instrument technicians' training is constantly updated to stay current with the latest gas analyser market trends.



Accreditation number: 19660

Table of Contents

Document Control	2
Distribution	2
Norditech Accreditations	2
Table of Contents	3
Figures	5
Tables	6
1. Executive Summary	8
2. Introduction	8
2.1 Project Background	8
2.2 Outlet Monitor Locations	9
3. Air Quality Limits	10
3.1 Standards Compliance	10
4. Explanation of Monitoring	11
4.1 Methodology.....	11
5. Data Validation and Reporting	12
5.1 Data Collection	12
5.2 Data Validation	12
5.3 Reporting and Calculations.....	13
5.3.1 Data Availability	14
5.3.2 Unit Conversions.....	14
6. Calibration and Maintenance	15
6.1 Units and Uncertainties	15
6.2 Automatic Instrument Calibration Checks.....	16
6.3 Last Calibration and Maintenance Records	16
6.3.1 October 2025.....	16
6.3.2 November 2025	17
6.3.3 December 2025	18
7. Results	19
7.1 Exceedances	19
7.2 Data Availability	21
7.3 Tabulated Results	22
7.3.1 Statistical Summary of 1-hour Mass Rate Data Western and Eastern Ventilation Stacks	22

7.4	Graphical Representations	25
7.4.1	Eastlink Ventilation Stack Outlet Monthly Charts	25
7.4.2	October 2025	25
7.4.2.1	October 2025 – Monthly 1-hour mass rate NO ₂	25
7.4.2.2	October 2025 – Monthly 1-hour mass rate NO	26
7.4.2.3	October 2025 – Monthly 1-hour mass rate CO	26
7.4.2.4	October 2025 – Monthly 1-hour mass rate PM _{2.5}	27
7.4.2.5	October 2025 – Monthly 1-hour mass rate PM ₁₀	27
7.4.2.6	October 2025 – Monthly 1-hour average stack velocity.....	28
7.4.2.7	October 2025 – Monthly 1-hour average stack temperature	28
7.4.3	November 2025	29
7.4.3.1	November 2025 – Monthly 1-hour mass rate NO ₂	29
7.4.3.2	November 2025 – Monthly 1-hour mass rate NO	29
7.4.3.3	November 2025 – Monthly 1-hour mass rate CO	30
7.4.3.4	November 2025 – Monthly 1-hour mass rate PM _{2.5}	30
7.4.3.5	November 2025 – Monthly 1-hour mass rate PM ₁₀	31
7.4.3.6	November 2025 – Monthly 1-hour average stack velocity	31
7.4.3.7	November 2025 – Monthly 1-hour average stack temperature.....	32
7.4.4	December 2025	32
7.4.4.1	December 2025 – Monthly 1-hour mass rate NO ₂	32
7.4.4.2	December 2025 – Monthly 1-hour mass rate NO	33
7.4.4.3	December 2025 – Monthly 1-hour mass rate CO	33
7.4.4.4	December 2025 – Monthly 1-hour mass rate PM _{2.5}	34
7.4.4.5	December 2025 – Monthly 1-hour mass rate PM ₁₀	34
7.4.4.6	December 2025 – Monthly 1-hour average stack velocity	35
7.4.4.7	December 2025 – Monthly 1-hour average stack temperature.....	35
8.	Data Exceptions	36
8.1	October 2025.....	36
8.1.1	October 2025 Western Ventilation Stack	36
8.1.2	October 2025 Eastern Ventilation Stack	37
8.2	November 2025	38
8.2.1	November 2025 Western Ventilation Stack	38
8.2.2	November 2025 Eastern Ventilation Stack.....	39
8.3	December 2025	40
8.3.1	December 2025 Western Ventilation Stack	40
8.3.2	December 2025 Eastern Ventilation Stack.....	41
9.	Report Summary.....	41
10.	Data validation explanations	41

Figures

Figure 1.Outlet monitoring location coordinates	9
Figure 2. October 2025 Monthly 1-hour mass rate NO ₂	25
Figure 3. October 2025 Monthly 1-hour mass rate NO.....	26
Figure 4. October 2025 Monthly 1-hour mass rate CO.....	26
Figure 5. October 2025 Monthly 1-hour mass rate PM _{2.5}	27
Figure 6. October 2025 Monthly 1-hour mass rate PM ₁₀	27
Figure 7. October 2025 Monthly 1-hour average stack velocity	28
Figure 8. October 2025 Monthly 1-hour average stack temperature	28
Figure 9. November 2025 Monthly 1-hour mass rate NO ₂	29
Figure 10. November 2025 Monthly 1-hour mass rate NO.....	29
Figure 11. November 2025 Monthly 1-hour mass rate CO	30
Figure 12. November 2025 Monthly 1-hour mass rate PM _{2.5}	30
Figure 13. November 2025 Monthly 1-hour mass rate PM ₁₀	31
Figure 14. November 2025 Monthly 1-hour average stack velocity.....	31
Figure 15. November 2025 Monthly 1-hour average stack temperature	32
Figure 16. December 2025 Monthly 1-hour mass rate NO ₂	32
Figure 17. December 2025 Monthly 1-hour mass rate NO.....	33
Figure 18. December 2025 Monthly 1-hour mass rate CO.....	33
Figure 19. December 2025 Monthly 1-hour mass rate PM _{2.5}	34
Figure 20. December 2025 Monthly 1-hour mass rate PM ₁₀	34
Figure 21. December 2025 Monthly 1-hour average stack velocity.....	35
Figure 22. December 2025 Monthly 1-hour average stack temperature	35

Tables

Table 1. Outlet Coordinates	9
Table 2. Ventilation Outlet Air Quality Limits	10
Table 3. Measurement methods and instrumentation.....	11
Table 4. Measurement units and uncertainties	15
Table 5. Daily Calibration Checks Times	16
Table 6. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – October	16
Table 7. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – October ...	17
Table 8. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – November	17
Table 9. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – November	18
Table 10. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – December.....	18
Table 11. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – December	19
Table 12. October 2025 Exceedances of EPA Goals.....	19
Table 13. November 2025 Exceedances of EPA Goals	20
Table 14. December 2025 Exceedances of EPA Goals	20
Table 15. October 2025 Data Availability	21
Table 16. November 2025 Data Availability	21
Table 17. December 2025 Data Availability	22
Table 18. October 2025 Summary Table	22
Table 19. November 2025 Summary Table	23
Table 20. December 2025 Summary Table	23
Table 21. October 2025 Percentile Summary of 1-hour mass rate pollutant data	23
Table 22. November 2025 Percentile Summary of 1-hour mass rate pollutant data	24
Table 23. December 2025 Percentile Summary of 1-hour mass rate pollutant data	24
Table 24. October 2025 Western Ventilation Stack data validation	36
Table 25. October 2025 Eastern Ventilation Stack data validation	37
Table 26. November 2025 Western Ventilation Stack data validation	38
Table 27. November 2025 Eastern Ventilation Stack data validation.....	39
Table 28. December 2025 Western Ventilation Stack data validation	40
Table 29. December 2025 Eastern Ventilation Stack data validation.....	41

Glossary

The following terms and abbreviations are used in this report

Abbreviation	Meaning
°C	Degrees Celsius
%	Percent
CO	Carbon monoxide
eq.	Equivalents
kPa	kilopascal
mg/m ³	Milligrams per cubic meter at dry, standard temperature and pressure (0°C and 101.3 kPa)
NO	Nitric oxide
NO ₂	Nitrogen dioxide
NO _x	Oxides of nitrogen
RH	Relative Humidity
PM10	Particles size ≤10µm
VOC	Volatile organic compounds
VSO	Ventilation Stack Outlet

1. Executive Summary

EastLink is a 39 km motorway running between Nunawading and Frankston, linking the Eastern, Monash Frankston and Peninsula Link freeways. Two 1.6 km tunnels pass under the Mullum Mullum Valley, with a ventilation stack at the end of each tunnel as an exit point for tunnel ventilation.

Two ventilation stacks provide ventilation for the tunnel, one at the western end of the tunnel at Discharge Point 1 (DP1), and one at the eastern end of the tunnel at Discharge Point 2 (DP2).

This report presents the monthly validated stack data for October 2025 to December 2025 to Ventia Pty Ltd for the EastLink Tunnel.

2. Introduction

2.1 Project Background

Norditech were contracted by Ventia Pty Ltd in August 2021 to provide continuous stack air quality monitoring and reporting services for the EastLink Tunnel. Ventia Pty Ltd are responsible for the operation and maintenance of the motorway.

Norditech is a NATA accredited organization (Accreditation Number: 19660)

Addresses of relevant parties:

Norditech Pty Ltd
2/87 Station Rd
Seven Hills NSW 2147

Ventia Pty Ltd
2 Hillcrest Avenue
Ringwood VIC 3134

This report presents the validated ventilation stack data for .

- Describe air quality measurements.
- Reports any readings above the Eastlink licence Limits.
- Compare monitoring results.
- It has been quality assured.

2.2 Outlet Monitor Locations

The locations of the EastLink Tunnel Western and Eastern ventilation stacks are detailed in Table 1 and **Error! Reference source not found.** below.

Location	Latitude	Longitude
Western Ventilation Stack	-37.801229°	145.196092°
Eastern Ventilation Stack	-37.808885°	145.212012°

Table 1. Outlet Coordinates

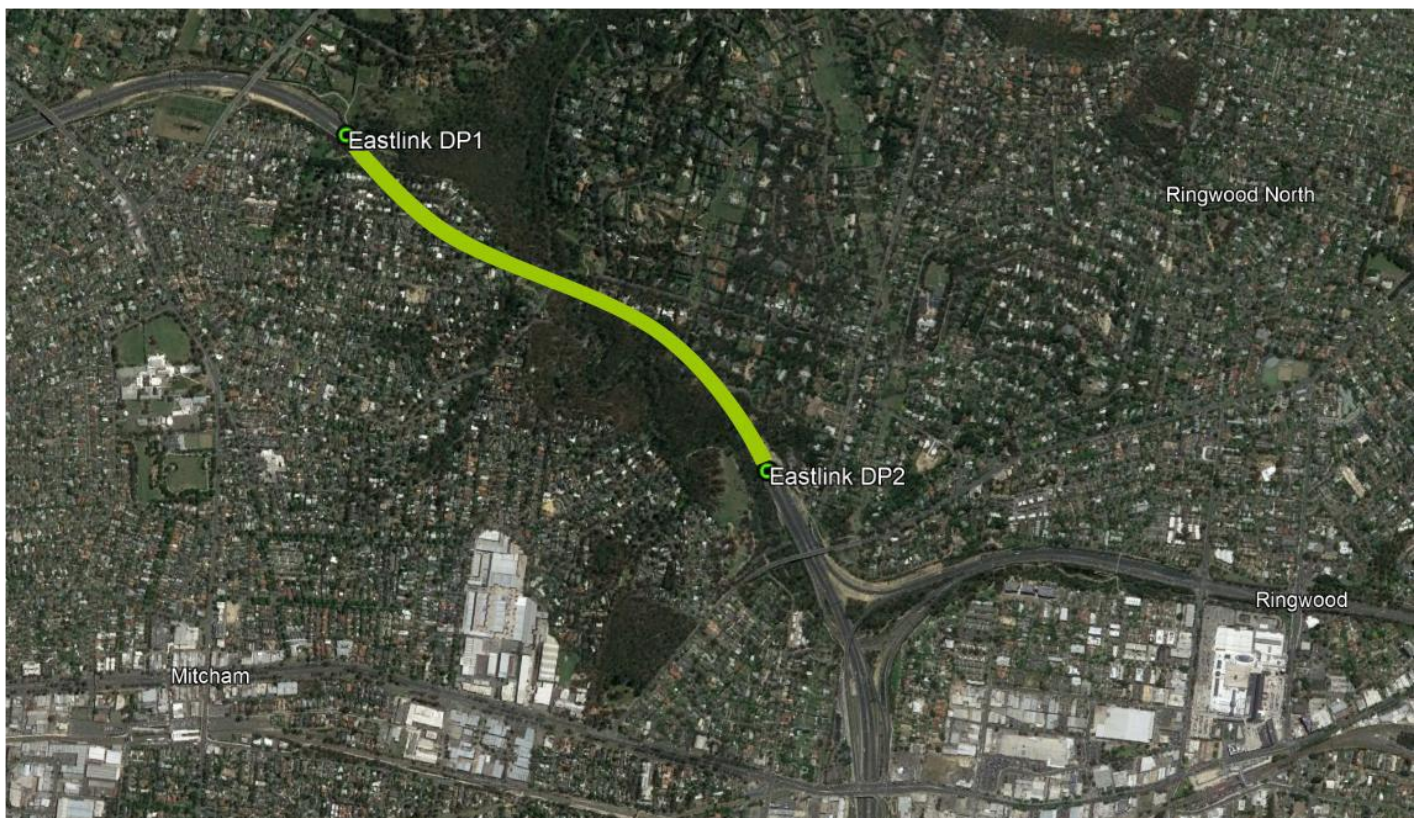


Figure 1. Outlet monitoring location coordinates

3. Air Quality Limits

Air quality limits are provided in Condition LI_DA1.13 of the Environment Protection Authority (Victoria) Licence No 2043 for the EastLink Tunnel. The air quality limits for 1-hour mass rates are shown in Table below.

Pollutant / Parameter	Type of Measurement	Concentration Limit	Unit
NO ₂	Average – 1 hour block	3.98	kg/h
CO	Average – 1 hour block	112	kg/h
PM _{2.5}	Average – 1 hour block	2.4	kg/h
PM ₁₀	Average – 1 hour block	2.6	kg/h

Table 2. Ventilation Outlet Air Quality Limits

The procedure for reporting particulate matter results from the TEOMs and assessment of licence compliance is detailed in the EastLink Particulate Matter Protocol (PMP) dated 17/06/2013. The PMP requires validated uncorrected TEOM one hour clock average data to be compared to the following TEOM mass rate compliance limits for both DP1 and DP2.

- PM2.5: 2.0 kg/h
- PM10: 2.0 kg/h

3.1 Standards Compliance

Norditech’s NATA Accreditation does not cover the following parameters monitored at the EastLink Tunnel ventilation stack air quality monitoring stations.

- Measurement of Stack Flow.
- AS/NZS 3580.9.8 refers specifically to the monitoring of PM10.

4. Explanation of Monitoring

4.1 Methodology

In the tunnel air is discharged via two ventilation stacks – one located at the Western end of the tunnel (DP1), and one located at the Eastern end (DP2). For each stack, monitoring as per the requirements of EPA Licence 2043 is undertaken.

Gaseous parameters are sampled by an extractive sampling system. Oxides of nitrogen are measured using chemiluminescence. Carbon monoxide is measured using non-dispersive infra-red absorption.

Particulates PM10 and PM2.5 are measured using tapered element oscillating microbalances.

Stack gas velocity is measured using an optical flow sensor.

Monthly routine maintenance is undertaken by Norditech. Maintenance is performed as per the relevant Australian Standard or in house method. Maintenance cycles generally involve 1, 3, 6 and 12 monthly scheduled items.

The following instrumentation and methods are used in data collection:

EastLink Ventilation Stack Measurement Methods		
Pollutant / Parameter	Method	Instrument
PM ₁₀	AS/NZS 3580.9.8	Thermo 1405 TEOM
	In house method TP.005	
	AS 4323.1	
PM _{2.5}	In house method TP.026	Thermo 1405 TEOM
	AS 4323.1	
NO	In house method TP.001	Thermo Scientific 42i
NO ₂	In house method TP.001	Thermo Scientific 42i
NO _x	In house method TP.001	Thermo Scientific 42i
CO	In house method TP.003	Thermo Scientific 48i
Temperature	In house method TP.012	PT100
Stack Velocity	USEAP (CFR 40) Part 75	Flowsic100

Table 3. Measurement methods and instrumentation

5. Data Validation and Reporting

5.1 Data Collection

At each Air Quality Monitoring Station, data is logged to an EnviDAS data logger at 1 minute average intervals. Each 1-minute average is calculated from data sampled at 10 second intervals.

Data is transferred automatically to Norditech's data collection software via a TCP/IP link over 4G cellular network, at a frequency of not less than 1-hour. Two datasets are maintained by Norditech, one for data validation and reporting purposes, and a non-validated data set for reference purposes.

5.2 Data Validation

Data validation is performed as per Norditech's data validation procedure TP.022. The data validation process identifies any data that is deemed not to be valid. This data is flagged as invalid in the database and is removed from the reported data.

Data may be deemed invalid for several reasons, including but not limited to:

- Instrument fault.
- Instrument calibration out of tolerance.
- Maintenance activities.

For further details and explanations of reasons for invalidating data, please refer to Section 12 – Data Validation Explanations.

Initial visual inspection of data is performed by inspection of graphs to identify any anomalies in the data set.

Site visit logs and maintenance and calibration certificates are cross referenced to the data set and any data affected by maintenance activities are flagged.

Instrument drift and calibration tolerances are checked, and data flagged in the database as necessary as per NATA compliance requirements.

5.3 Reporting and Calculations

All calculations and averages are calculated from 1 minute average base data and are reported as 'end time' when the averaging periods of eight hours or less. IE the average data for 01:00 is the data from 00:00 through to 01:00. One-hour averages are calculated based on a clock hour. One day averages are calculated based on calendar days. All averages are based on a minimum of 75% valid readings within the averaging period.

All data is reported at Australian Eastern Standard Time.

Validated data for Quarter 1 Month 1 is presented in the Excel workbook named "202510 EastLink Q4M1 Validated data.xlsx"

The workbooks each consist of the following sheets:

- Sheet 1: Cover
- Sheet 2: M1 Data kg1h – Hourly data in kg/h
- Sheet 3: M1 Data g5m – 5-minute data in grams/5m
- Sheet 4: M1 Data mgm3 1h – 1-hour data in mg/m3
- Sheet 5: M1 Data mgm3 5m – 5-minute data in mg/m3
- Sheet 6: Eastern Validation Data
- Sheet 7: Western Validation Data
-

Validated data for Quarter 1 Month 2 is presented in the Excel workbook named "202511 EastLink Q4M2 Validated data.xlsx"

The workbooks each consist of the following sheets:

- Sheet 1: Cover
- Sheet 2: M2 Data kg1h – Hourly data in kg/h
- Sheet 3: M2 Data g5m – 5-minute data in grams/5m
- Sheet 4: M2 Data mgm3 1h – 1-hour data in mg/m3
- Sheet 5: M2 Data mgm3 5m – 5-minute data in mg/m3
- Sheet 6: Eastern Validation Data
- Sheet 7: Western Validation Data

Validated data for Quarter 1 Month 3 is presented in the Excel workbook named “202512 EastLink Q4M3 Validated data.xlsx”

The workbook consists of the following sheets:

- Sheet 1: Cover
- Sheet 2: M3 Data kg1h – Hourly data in kg/h
- Sheet 3: M3 Data g5m – 5-minute data in grams/5m
- Sheet 4: M3 Data mgm3 1h – 1-hour data in mg/m3
- Sheet 5: M3 Data mgm3 5m – 5-minute data in mg/m3
- Sheet 6: Eastern Validation Data
- Sheet 7: Western Validation Data

5.3.1 Data Availability

Data availability refers to the amount of available data for the reporting period. Data availability is calculated using the following formula:

$$\text{Data availability \%} = \frac{\text{sum of available data points}}{\text{sum of possible data points}} * 100$$

Where:

- Sum of available data points is the number of validated 1-hour average data points for the reporting period
- Sum of possible data points is the number of theoretically available data points for the reporting period

5.3.2 Unit Conversions

Stack velocity readings are converted to flow rate using the following stack areas:

- Western Stack area 35 m²
- Eastern Stack area 35 m²

Pollutant and flow data are reported at actual conditions.

6. Calibration and Maintenance

6.1 Units and Uncertainties

EastLink Ventilation Stack Instrument Units and Uncertainties				
Parameter	Units	Resolution	Uncertainty	Measurement Range
CO	mg/m ³	0.01	± 8.2% of reading at 62.5mg/m ³ (k=1.96)	0 to 200
NO	mg/m ³	0.01	± 8.1% of reading for range 25.7 – 32.8mg/m ³ (k=1.96)	0 to 150
NO ₂	mg/m ³	0.01	± 8.5% of reading at 25.7mg/m ³ (k=1.96)	0 to 150
NO _x	mg/m ³	0.01	± 8.1% of reading for range 25.7 – 32.8mg/m ³ (k=1.96)	0 to 150
PM ₁₀	µg/m ³	0.1	±5.0 µg/m ³ or 3.6% of reading, whichever is the greater. (k=1.96)	0 to 5000
PM _{2.5}	µg/m ³	0.1	±5.0 µg/m ³ or 3.6% of reading, whichever is the greater. (k=1.96)	0 to 5000
Temperature	°C	0.1	±2.0 °C ¹	-25 to 105
Stack Velocity	m/s	1	±0.1 m/s ¹	-40 to +40

Table 4. Measurement units and uncertainties

¹ Manufacturer's stated accuracy

6.2 Automatic Instrument Calibration Checks

Table 5 below identifies the times at which the daily gaseous parameter automatic span and zero checks are performed.

This data is removed from the dataset, however, are not included in the data validation tables of data.

Location	Parameters	Daily Calibration Checks Times
Western (to 25/07/2024)	CO	00:00 - 00:34
	NO, NO ₂	01:00 - 01:44
Western (from 26/07/2024)	CO	01:00 - 01:44
	NO, NO ₂	
Eastern	CO	01:34 - 02:13
	NO, NO ₂	

Table 5. Daily Calibration Checks Times

6.3 Last Calibration and Maintenance Records

6.3.1 October 2025

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – October 2025			
Western Ventilation Stack (Discharge Point 1)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	21/10/2025	1 Monthly	21/10/2025
NO/NO ₂	21/10/2025	1 Monthly	21/10/2025
PM _{2.5}	16/09/2025	3 Monthly	16/09/2025
PM ₁₀	16/09/2025	3 Monthly	16/09/2025
Temperature	16/06/2025	12 Monthly	16/06/2025
Stack Velocity	25/08/2025	12 Monthly	25/08/2025

Table 6. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – October

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – October 2025			
East Ventilation Stack (Discharge Point 2)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	21/10/2025	1 Monthly	21/10/2025
NO/NO ₂	21/10/2025	1 Monthly	21/10/2025
PM _{2.5}	16/09/2025	3 Monthly	16/09/2025
PM ₁₀	16/09/2025	3 Monthly	16/09/2025
Temperature	16/06/2025	12 Monthly	16/06/2025
Stack Velocity	27/08/2025	12 Monthly	27/08/2025

Table 7. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – October

6.3.2 November 2025

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – November 2025			
Western Ventilation Stack (Discharge Point 1)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	21/11/2025	1 Monthly	21/11/2025
NO/NO ₂	21/11/2025	1 Monthly	21/11/2025
PM _{2.5}	16/09/2025	3 Monthly	16/09/2025
PM ₁₀	16/09/2025	3 Monthly	16/09/2025
Temperature	16/06/2025	12 Monthly	16/06/2025
Stack Velocity	25/08/2025	12 Monthly	25/08/2025

Table 8. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – November

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – November 2025			
East Ventilation Stack (Discharge Point 2)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	21/11/2025	1 Monthly	21/11/2025
NO/NO ₂	21/11/2025	1 Monthly	21/11/2025
PM _{2.5}	16/09/2025	3 Monthly	16/09/2025
PM ₁₀	16/09/2025	3 Monthly	16/09/2025
Temperature	16/06/2025	12 Monthly	16/06/2025
Stack Velocity	27/08/2025	12 Monthly	27/08/2025

Table 9. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – November

6.3.3 December 2025

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – December 2025			
Western Ventilation Stack (Discharge Point 1)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	16/12/2025	6 Monthly	16/12/2025
NO/NO ₂	16/12/2025	6 Monthly	16/12/2025
PM _{2.5}	16/12/2025	6 Monthly	16/12/2025
PM ₁₀	16/12/2025	6 Monthly	16/12/2025
Temperature	16/12/2025	6 Monthly	16/12/2025
Stack Velocity	25/08/2025	12 Monthly	25/08/2025

Table 10. Last Scheduled Maintenance and Calibration Dates - Western Ventilation Stack (Discharge Point 1) – December

EastLink Ventilation Stack Maintenance and Last Scheduled Calibration Dates – December 2025			
East Ventilation Stack (Discharge Point 2)			
Sensor	Date of Last Scheduled Maintenance	Maintenance Type	Date of Last Scheduled Calibration
CO	16/12/2025	6 Monthly	16/12/2025
NO/NO ₂	16/12/2025	6 Monthly	16/12/2025
PM _{2.5}	16/12/2025	6 Monthly	16/12/2025
PM ₁₀	16/12/2025	6 Monthly	16/12/2025
Temperature	16/12/2025	6 Monthly	16/12/2025
Stack Velocity	27/08/2025	12 Monthly	27/08/2025

Table 11. Last Scheduled Maintenance and Calibration Dates - East Ventilation Stack (Discharge Point 2) – December

7. Results

7.1 Exceedances

Instances of the ventilation stack pollutants exceeding the EPA Limits goals during the reporting period are presented in Table 12, Table 13, and Table 14 below. Maximum mass rates are provided for comparison to the limits.

There were nil exceedances of the prescribed limits during the reporting period.

EastLink Ventilation Stack Air Quality Limit Exceedances October 2025								
Location	Parameter	Time Period	Licence Limit	Units	Maximum Mass Rate	Number of exceedances	Value of Exceedance	Date and Time of exceedance
Western Ventilation Stack (Discharge Point 1)	NO ₂	1-hour	3.98	kg/h	0.41	-	-	-
	CO	1-hour	112	kg/h	3.81	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.13	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	0.41	-	-	-
Eastern Ventilation Stack (Discharge Point 2)	NO ₂	1-hour	3.98	kg/h	0.64	-	-	-
	CO	1-hour	112	kg/h	5.39	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.18	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	0.49	-	-	-

Table 12. October 2025 Exceedances of EPA Goals

EastLink Ventilation Stack Air Quality Limit Exceedances November 2025								
Location	Parameter	Time Period	Licence Limit	Units	Maximum Mass Rate	Number of exceedances	Value of Exceedance	Date and Time of exceedance
Western Ventilation Stack (Discharge Point 1)	NO ₂	1-hour	3.98	kg/h	0.38	-	-	-
	CO	1-hour	112	kg/h	3.89	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.16	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	0.37	-	-	-
Eastern Ventilation Stack (Discharge Point 2)	NO ₂	1-hour	3.98	kg/h	0.52	-	-	-
	CO	1-hour	112	kg/h	5.41	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.22	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	1.03	-	-	-

Table 13. November 2025 Exceedances of EPA Goals

EastLink Ventilation Stack Air Quality Limit Exceedances December 2025								
Location	Parameter	Time Period	Licence Limit	Units	Maximum Mass Rate	Number of exceedances	Value of Exceedance	Date and Time of exceedance
Western Ventilation Stack (Discharge Point 1)	NO ₂	1-hour	3.98	kg/h	0.42	-	-	-
	CO	1-hour	112	kg/h	4.45	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.16	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	0.44	-	-	-
Eastern Ventilation Stack (Discharge Point 2)	NO ₂	1-hour	3.98	kg/h	0.71	-	-	-
	CO	1-hour	112	kg/h	6.84	-	-	-
	PM _{2.5}	1-hour	2.4	kg/h	0.16	-	-	-
	PM ₁₀	1-hour	2.6	kg/h	0.43	-	-	-

Table 14. December 2025 Exceedances of EPA Goals

7.2 Data Availability

Data availability for the ventilation stack outlet sensors is provided in the table below.

EastLink Ventilation Stack Data Availability October 2025								
Station	Parameter	NO	NO ₂	CO	PM _{2.5}	PM ₁₀	Stack Velocity	Stack Temperature
Western	Data Availability	88.3%	88.3%	95.4%	99.9%	100.0%	100.0%	100.0%
	Collected Periods	657.0	657.0	710.0	743.0	744.0	744.0	744.0
	Available Periods	744.0	744.0	744.0	744.0	744.0	744.0	744.0
Eastern	Data Availability	95.6%	95.6%	95.3%	99.2%	98.4%	100.0%	100.0%
	Collected Periods	711.0	711.0	709.0	738.0	732.0	744.0	744.0
	Available Periods	744.0	744.0	744.0	744.0	744.0	744.0	744.0

Table 15. October 2025 Data Availability

EastLink Ventilation Stack Data Availability November 2025								
Station	Parameter	NO	NO ₂	CO	PM _{2.5}	PM ₁₀	Stack Velocity	Stack Temperature
Western	Data Availability	95.3%	95.3%	95.3%	98.3%	99.7%	100.0%	100.0%
	Collected Periods	686.0	686.0	686.0	708.0	718.0	720.0	720.0
	Available Periods	720.0	720.0	720.0	720.0	720.0	720.0	720.0
Eastern	Data Availability	95.3%	95.3%	92.4%	98.5%	98.2%	100.0%	100.0%
	Collected Periods	686.0	686.0	665.0	709.0	707.0	720.0	720.0
	Available Periods	720.0	720.0	720.0	720.0	720.0	720.0	720.0

Table 16. November 2025 Data Availability

EastLink Ventilation Stack Data Availability December 2025								
Station	Parameter	NO	NO ₂	CO	PM _{2.5}	PM ₁₀	Stack Velocity	Stack Temperature
Western	Data Availability	91.0%	91.0%	92.6%	99.3%	98.9%	100.0%	100.0%
	Collected Periods	677.0	677.0	689.0	739.0	736.0	744.0	744.0
	Available Periods	744.0	744.0	744.0	744.0	744.0	744.0	744.0
Eastern	Data Availability	95.4%	95.4%	95.3%	98.9%	99.2%	100.0%	100.0%
	Collected Periods	710.0	710.0	709.0	736.0	738.0	744.0	744.0
	Available Periods	744.0	744.0	744.0	744.0	744.0	744.0	744.0

Table 17. December 2025 Data Availability

Remarks: Data Availability is calculated with 1 hour average data

7.3 Tabulated Results

7.3.1 Statistical Summary of 1-hour Mass Rate Data Western and Eastern Ventilation Stacks

Table 18 presents 1-hour mass rate statistical data for the Western and Eastern ventilation stacks.

1-hour mass rates are calculated from 1 minute average data.

EastLink Ventilation Stack Summary October 2025					
Location	Parameter	1hr Average Maximum	1hr Average Minimum	Monthly Average	Monthly Total
Western Ventilation Stack	NO (kg/h)	2.53	0.00	0.48	314.44
	NO ₂ (kg/h)	0.41	0.00	0.09	62.08
	CO (kg/h)	3.81	0.00	1.09	777.07
	PM _{2.5} (kg/h)	0.13	0.00	0.03	19.70
	PM ₁₀ (kg/h)	0.41	0.00	0.05	39.92
Eastern Ventilation Stack	NO (kg/h)	3.35	0.00	0.79	564.38
	NO ₂ (kg/h)	0.64	0.00	0.14	98.73
	CO (kg/h)	5.39	0.00	1.37	974.04
	PM _{2.5} (kg/h)	0.18	0.00	0.04	26.49
	PM ₁₀ (kg/h)	0.49	0.00	0.09	65.44

Table 18. October 2025 Summary Table

EastLink Ventilation Stack Summary November 2025					
Location	Parameter	1hr Average Maximum	1hr Average Minimum	Monthly Average	Monthly Total
Western Ventilation Stack	NO (kg/h)	2.37	0.00	0.43	293.94
	NO ₂ (kg/h)	0.38	0.00	0.08	57.50
	CO (kg/h)	3.89	0.00	1.07	731.26
	PM _{2.5} (kg/h)	0.16	0.00	0.03	18.16
	PM ₁₀ (kg/h)	0.37	0.00	0.05	34.61
Eastern Ventilation Stack	NO (kg/h)	3.34	0.00	0.70	482.93
	NO ₂ (kg/h)	0.52	0.00	0.12	81.06
	CO (kg/h)	5.41	0.00	1.25	828.82
	PM _{2.5} (kg/h)	0.22	0.00	0.03	23.82
	PM ₁₀ (kg/h)	1.03	0.00	0.07	52.49

Table 19. November 2025 Summary Table

EastLink Ventilation Stack Summary December 2025					
Location	Parameter	1hr Average Maximum	1hr Average Minimum	Monthly Average	Monthly Total
Western Ventilation Stack	NO (kg/h)	3.31	0.00	0.41	278.44
	NO ₂ (kg/h)	0.42	0.00	0.08	53.24
	CO (kg/h)	4.45	0.00	1.08	746.52
	PM _{2.5} (kg/h)	0.16	0.00	0.03	20.25
	PM ₁₀ (kg/h)	0.44	0.00	0.05	37.25
Eastern Ventilation Stack	NO (kg/h)	3.44	0.00	0.67	474.14
	NO ₂ (kg/h)	0.71	0.00	0.12	82.86
	CO (kg/h)	6.84	0.00	1.30	925.19
	PM _{2.5} (kg/h)	0.16	0.00	0.03	23.49
	PM ₁₀ (kg/h)	0.43	0.00	0.08	56.25

Table 20. December 2025 Summary Table

EastLink Ventilation Stack Percentile Summary October 2025								
Location	Parameter	Maximum	99 th Percentile	98 th Percentile	95 th Percentile	90 th Percentile	75 th Percentile	50 th Percentile
Western Ventilation Stack	NO (kg/h)	2.53	2.17	2.00	1.58	1.10	0.76	0.36
	NO ₂ (kg/h)	0.41	0.35	0.33	0.25	0.19	0.15	0.10
	CO (kg/h)	3.81	3.28	3.00	2.67	2.34	1.77	1.26
	PM _{2.5} (kg/h)	0.13	0.10	0.10	0.08	0.06	0.04	0.03
	PM ₁₀ (kg/h)	0.41	0.28	0.24	0.17	0.11	0.08	0.05
Eastern Ventilation Stack	NO (kg/h)	3.35	2.93	2.72	2.34	2.04	1.51	0.49
	NO ₂ (kg/h)	0.64	0.50	0.47	0.41	0.35	0.23	0.12
	CO (kg/h)	5.39	4.56	4.35	3.69	3.07	2.26	1.52
	PM _{2.5} (kg/h)	0.18	0.15	0.13	0.11	0.09	0.07	0.03
	PM ₁₀ (kg/h)	0.49	0.43	0.35	0.29	0.22	0.15	0.07

Table 21. October 2025 Percentile Summary of 1-hour mass rate pollutant data

EastLink Ventilation Stack Percentile Summary November 2025								
Location	Parameter	Maximum	99 th Percentile	98 th Percentile	95 th Percentile	90 th Percentile	75 th Percentile	50 th Percentile
Western Ventilation Stack	NO (kg/h)	2.37	2.13	1.93	1.43	1.06	0.70	0.30
	NO ₂ (kg/h)	0.38	0.33	0.31	0.22	0.18	0.13	0.08
	CO (kg/h)	3.89	3.37	3.22	2.82	2.38	1.75	1.19
	PM _{2.5} (kg/h)	0.16	0.12	0.11	0.08	0.06	0.04	0.02
	PM ₁₀ (kg/h)	0.37	0.29	0.25	0.15	0.10	0.08	0.04
Eastern Ventilation Stack	NO (kg/h)	3.34	2.92	2.72	2.38	1.95	1.38	0.41
	NO ₂ (kg/h)	0.52	0.49	0.45	0.38	0.29	0.20	0.09
	CO (kg/h)	5.41	4.63	4.15	3.58	2.74	2.02	1.27
	PM _{2.5} (kg/h)	0.22	0.16	0.13	0.11	0.09	0.06	0.02
	PM ₁₀ (kg/h)	1.03	0.35	0.32	0.26	0.19	0.13	0.04

Table 22. November 2025 Percentile Summary of 1-hour mass rate pollutant data

EastLink Ventilation Stack Percentile Summary December 2025								
Location	Parameter	Maximum	99 th Percentile	98 th Percentile	95 th Percentile	90 th Percentile	75 th Percentile	50 th Percentile
Western Ventilation Stack	NO (kg/h)	3.31	2.08	1.94	1.41	1.07	0.59	0.30
	NO ₂ (kg/h)	0.42	0.35	0.30	0.24	0.18	0.12	0.08
	CO (kg/h)	4.45	3.62	3.39	2.97	2.49	1.77	1.18
	PM _{2.5} (kg/h)	0.16	0.13	0.12	0.10	0.07	0.04	0.02
	PM ₁₀ (kg/h)	0.44	0.29	0.26	0.17	0.12	0.07	0.04
Eastern Ventilation Stack	NO (kg/h)	3.44	3.08	2.83	2.46	1.93	1.03	0.41
	NO ₂ (kg/h)	0.71	0.57	0.51	0.42	0.29	0.18	0.09
	CO (kg/h)	6.84	4.94	4.53	3.90	3.02	2.09	1.37
	PM _{2.5} (kg/h)	0.16	0.14	0.13	0.11	0.09	0.05	0.02
	PM ₁₀ (kg/h)	0.43	0.37	0.33	0.28	0.21	0.11	0.06

Table 23. December 2025 Percentile Summary of 1-hour mass rate pollutant data

7.4 Graphical Representations

7.4.1 Eastlink Ventilation Stack Outlet Monthly Charts

The following charts present ventilation stack outlet data for CO, NO_x, VOC, PM10, Stack Temperature, Stack Pressure, Stack Velocity and Stack Moisture for Eastlink.

1-hour Averages are calculated from 1 minute average data.

7.4.2 October 2025

7.4.2.1 October 2025 – Monthly 1-hour mass rate NO₂

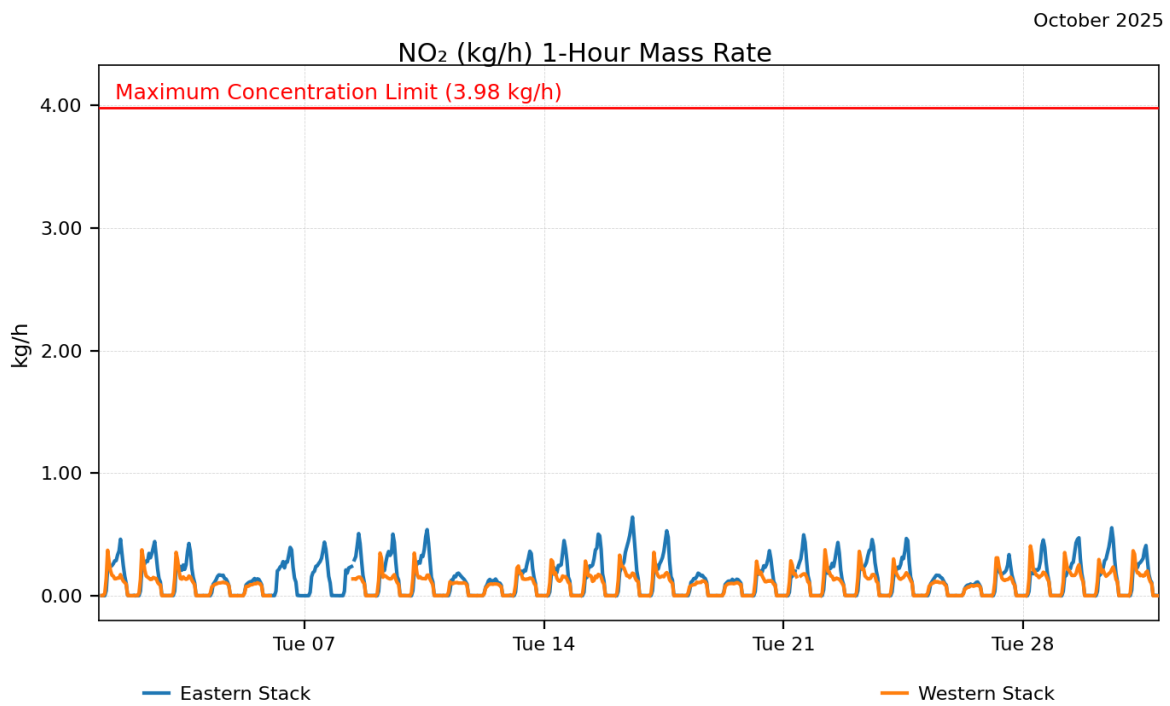


Figure 2. October 2025 Monthly 1-hour mass rate NO₂

7.4.2.2 October 2025 – Monthly 1-hour mass rate NO

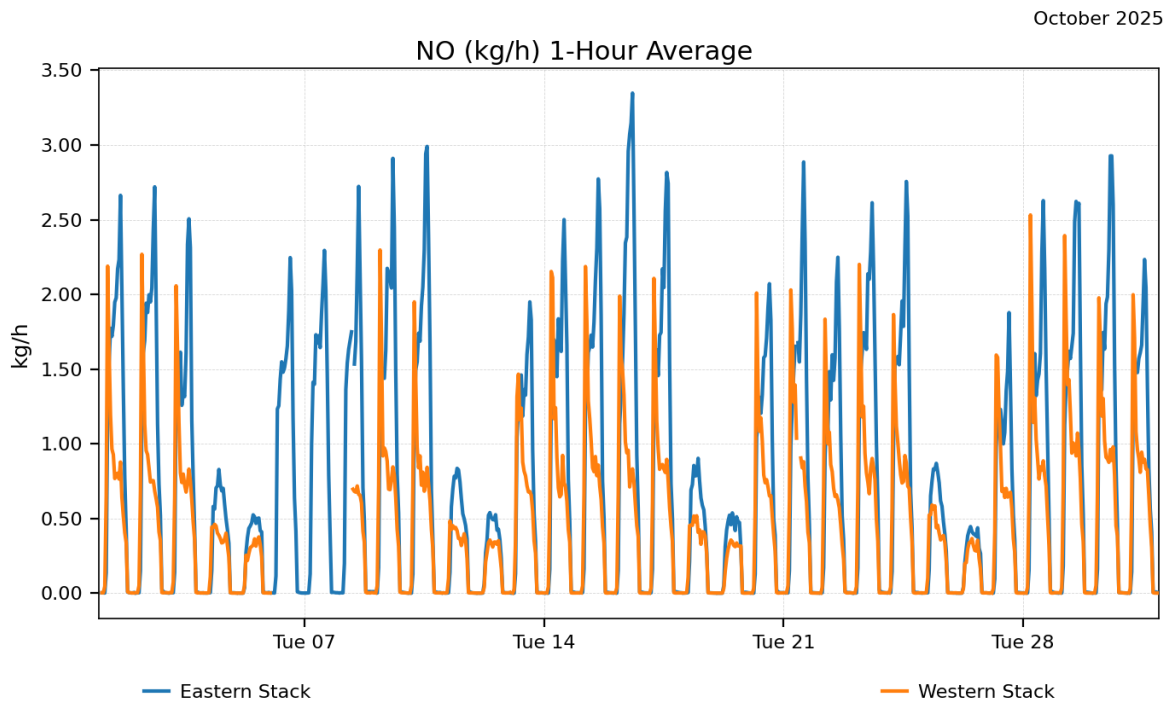


Figure 3. October 2025 Monthly 1-hour mass rate NO

7.4.2.3 October 2025 – Monthly 1-hour mass rate CO

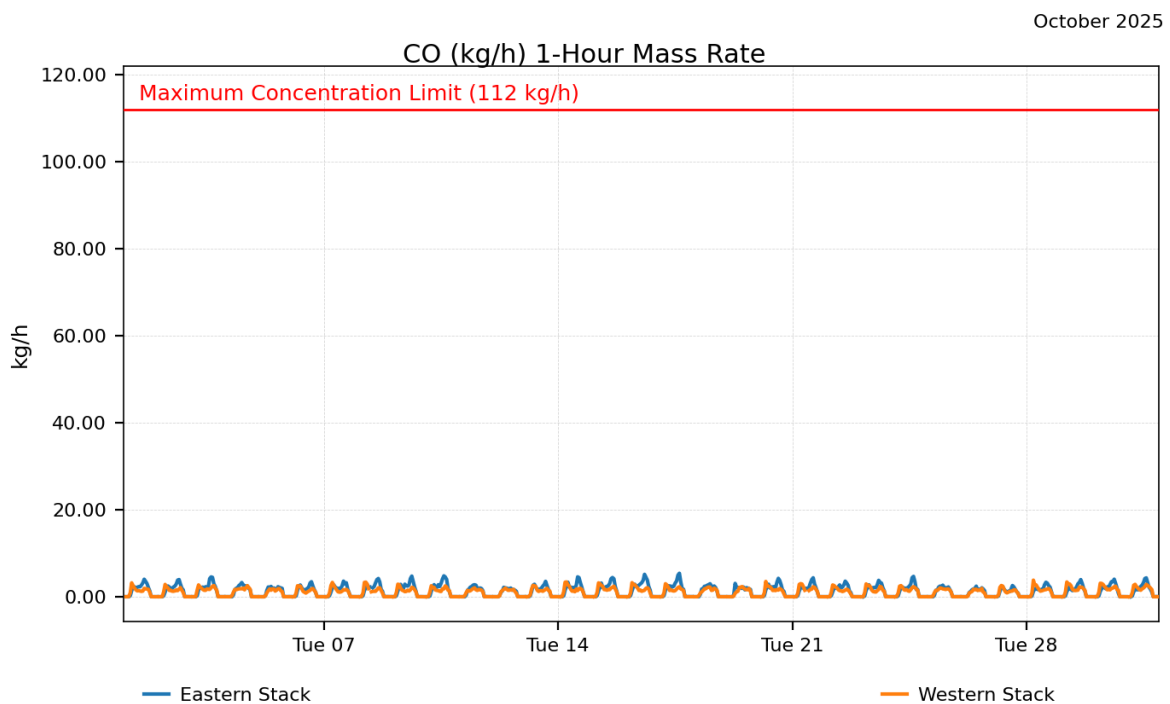


Figure 4. October 2025 Monthly 1-hour mass rate CO

7.4.2.4 October 2025 – Monthly 1-hour mass rate PM_{2.5}

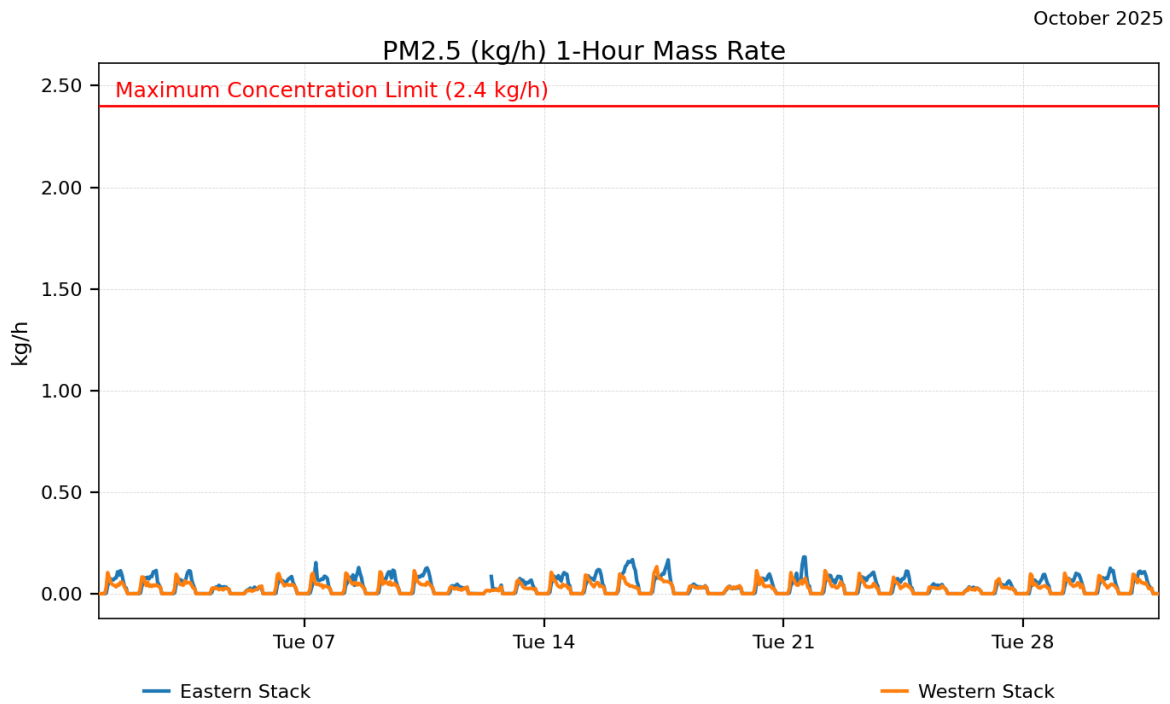


Figure 5. October 2025 Monthly 1-hour mass rate PM_{2.5}

7.4.2.5 October 2025 – Monthly 1-hour mass rate PM₁₀

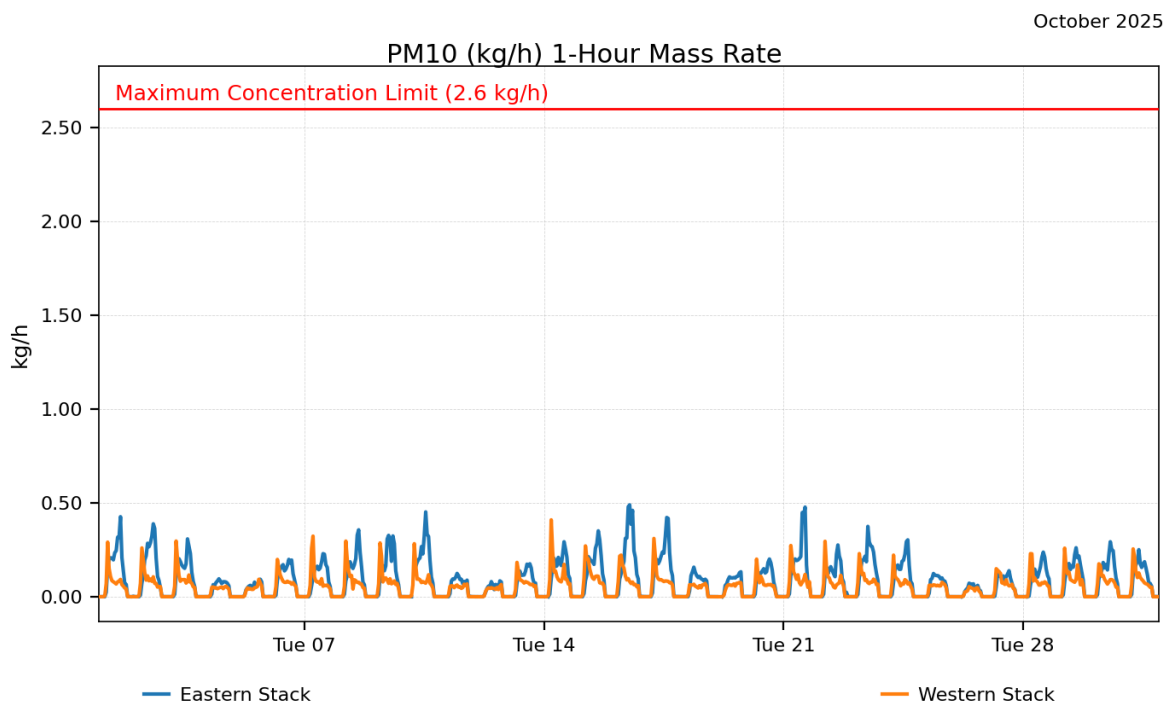


Figure 6. October 2025 Monthly 1-hour mass rate PM₁₀

7.4.2.6 October 2025 – Monthly 1-hour average stack velocity

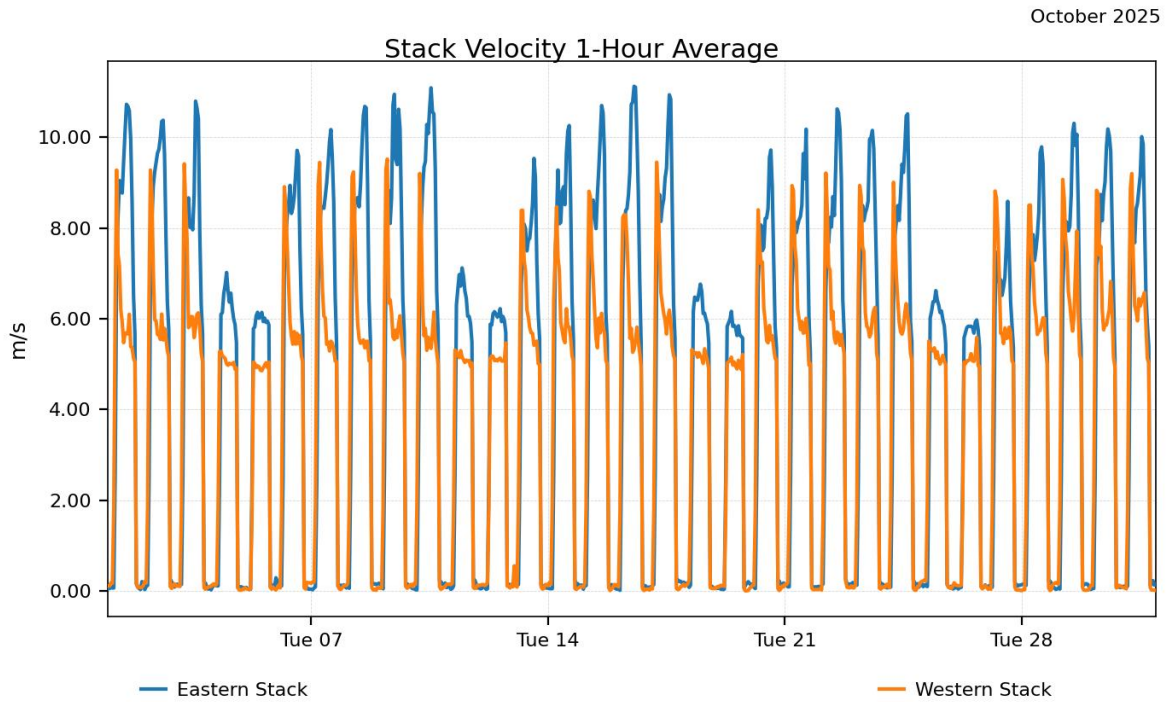


Figure 7. October 2025 Monthly 1-hour average stack velocity

7.4.2.7 October 2025 – Monthly 1-hour average stack temperature

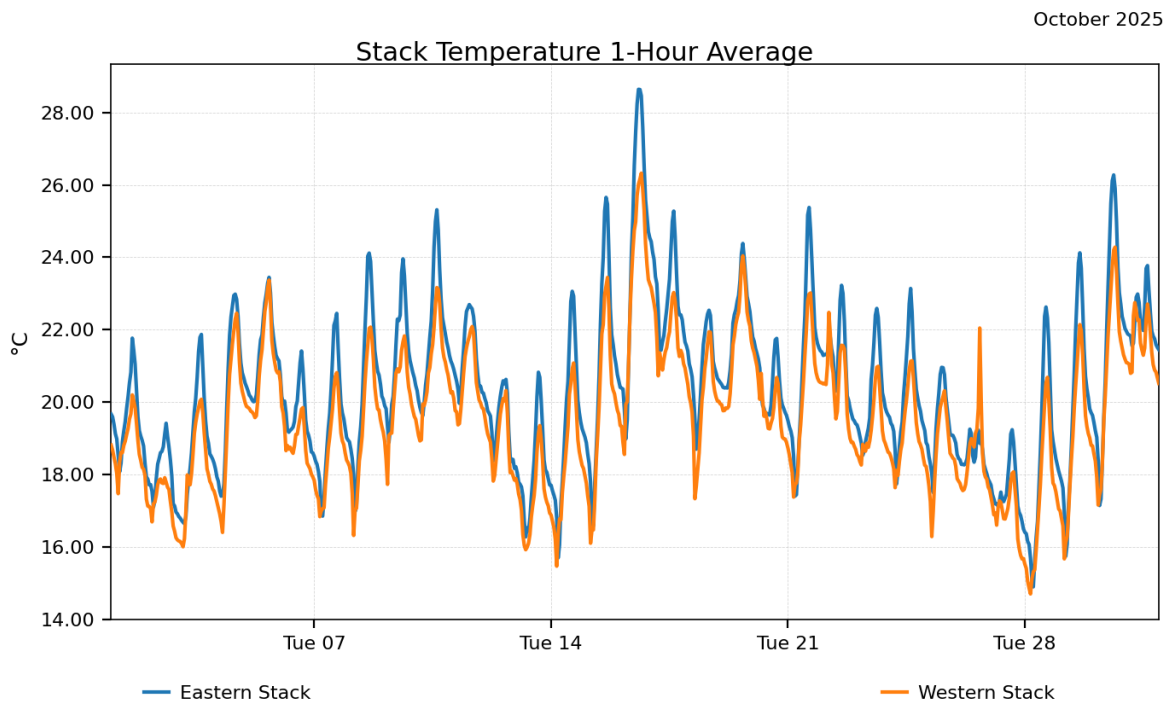


Figure 8. October 2025 Monthly 1-hour average stack temperature

7.4.3 November 2025

7.4.3.1 November 2025 – Monthly 1-hour mass rate NO₂

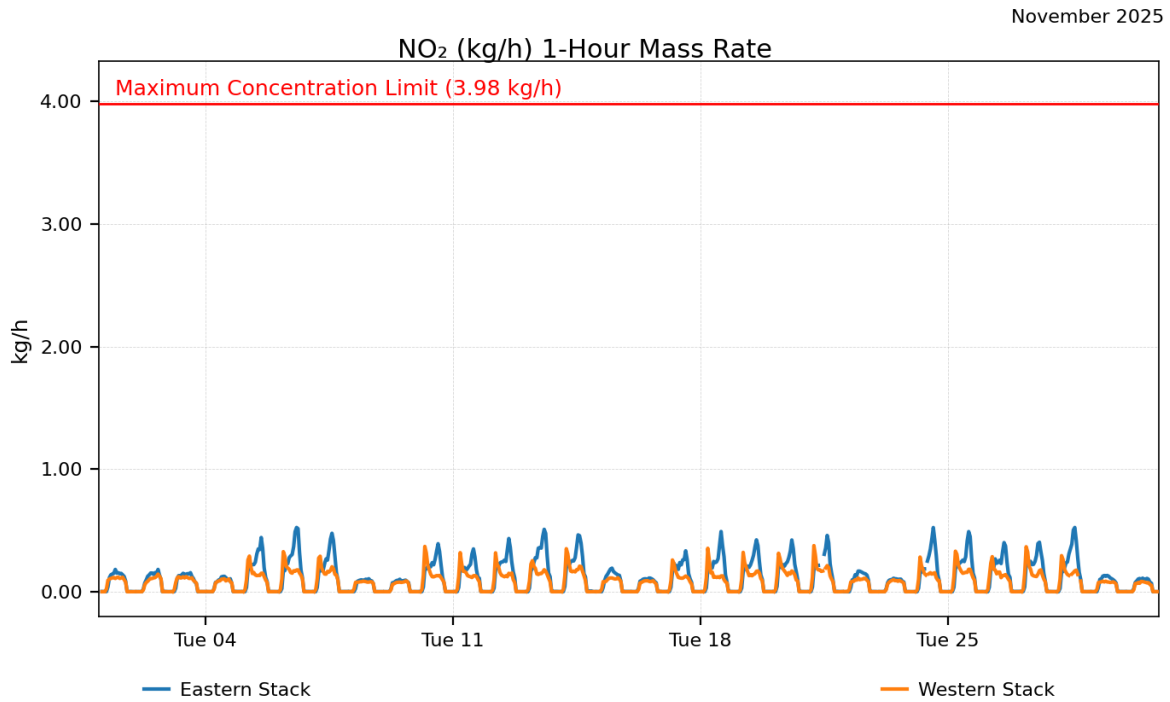


Figure 9. November 2025 Monthly 1-hour mass rate NO₂

7.4.3.2 November 2025 – Monthly 1-hour mass rate NO

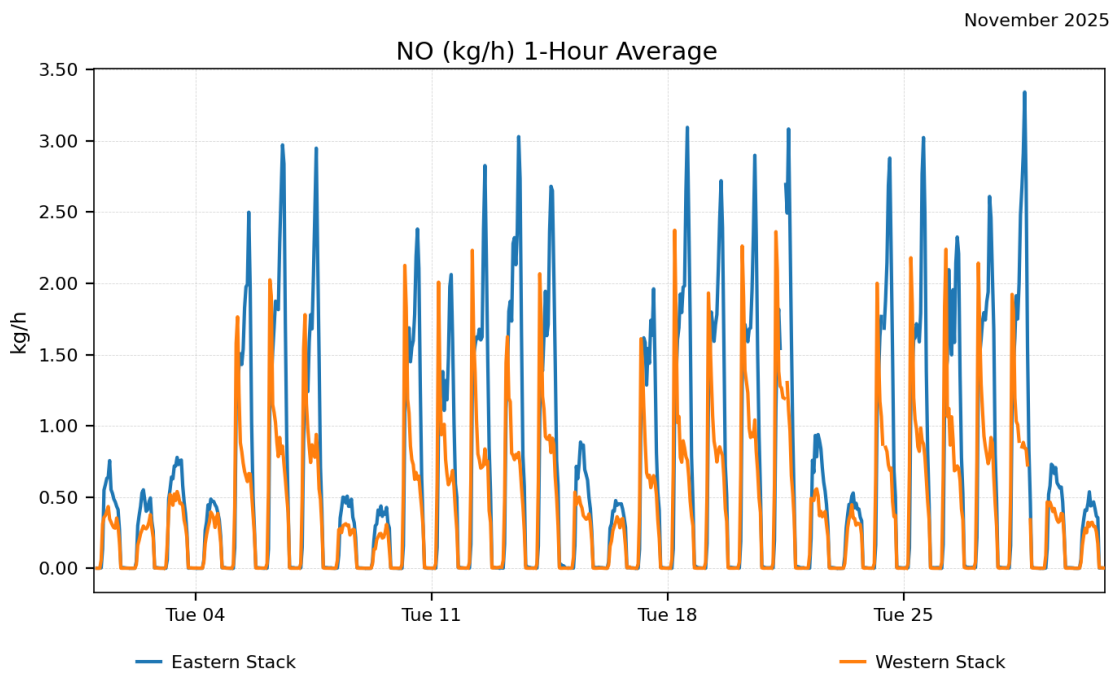


Figure 10. November 2025 Monthly 1-hour mass rate NO

7.4.3.3 November 2025 – Monthly 1-hour mass rate CO

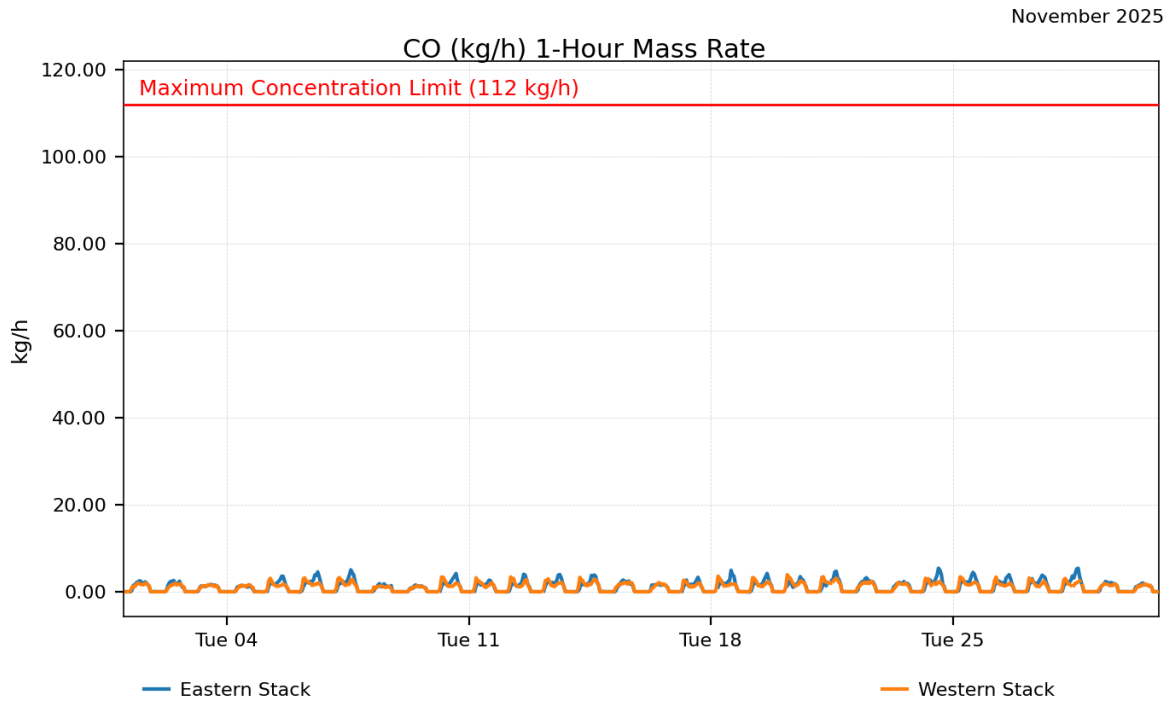


Figure 11. November 2025 Monthly 1-hour mass rate CO

7.4.3.4 November 2025 – Monthly 1-hour mass rate PM_{2.5}

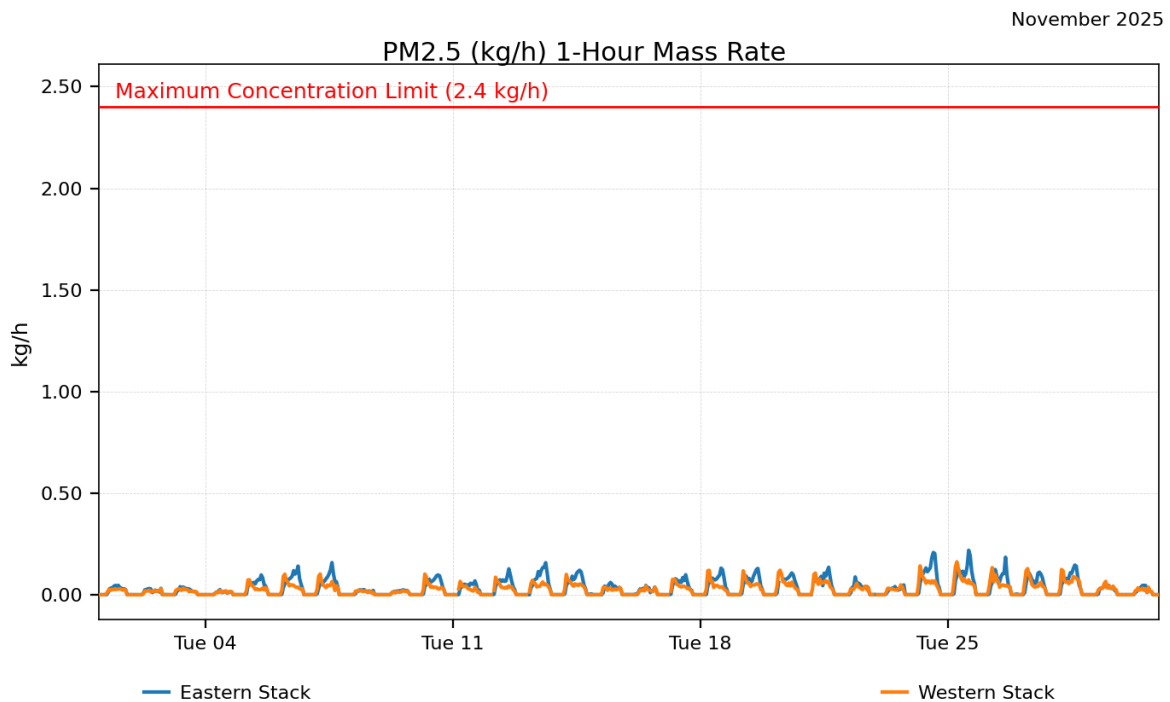


Figure 12. November 2025 Monthly 1-hour mass rate PM_{2.5}

7.4.3.5 November 2025 – Monthly 1-hour mass rate PM₁₀

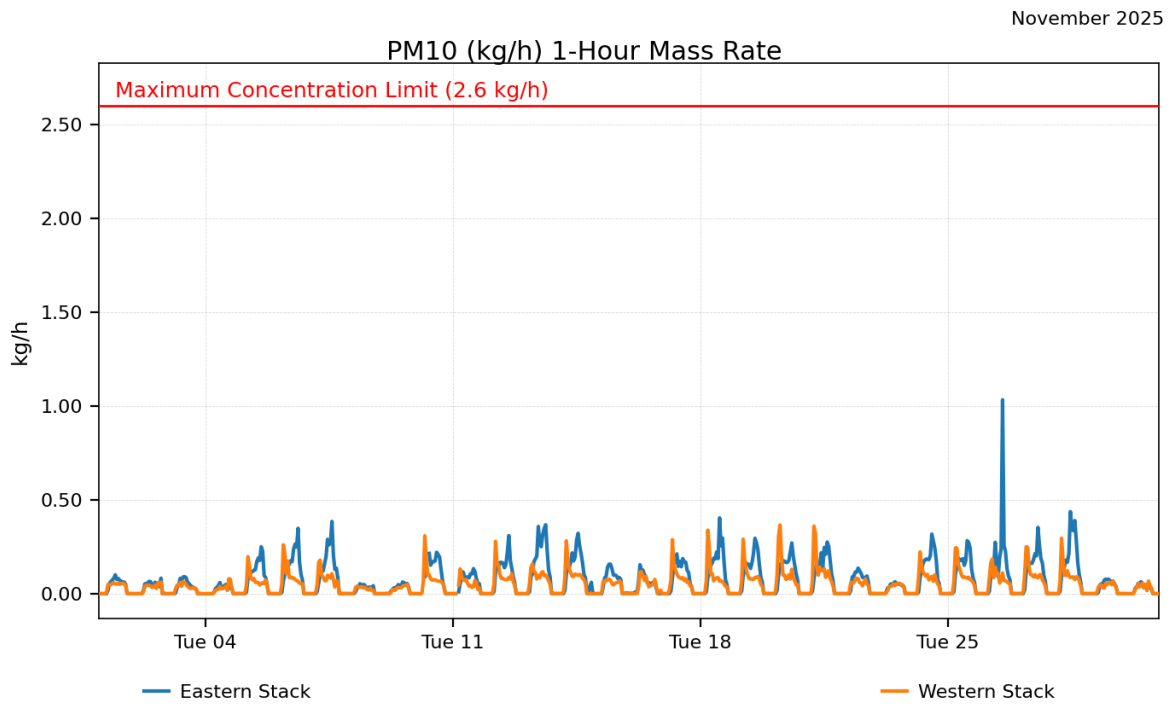


Figure 13. November 2025 Monthly 1-hour mass rate PM₁₀

7.4.3.6 November 2025 – Monthly 1-hour average stack velocity

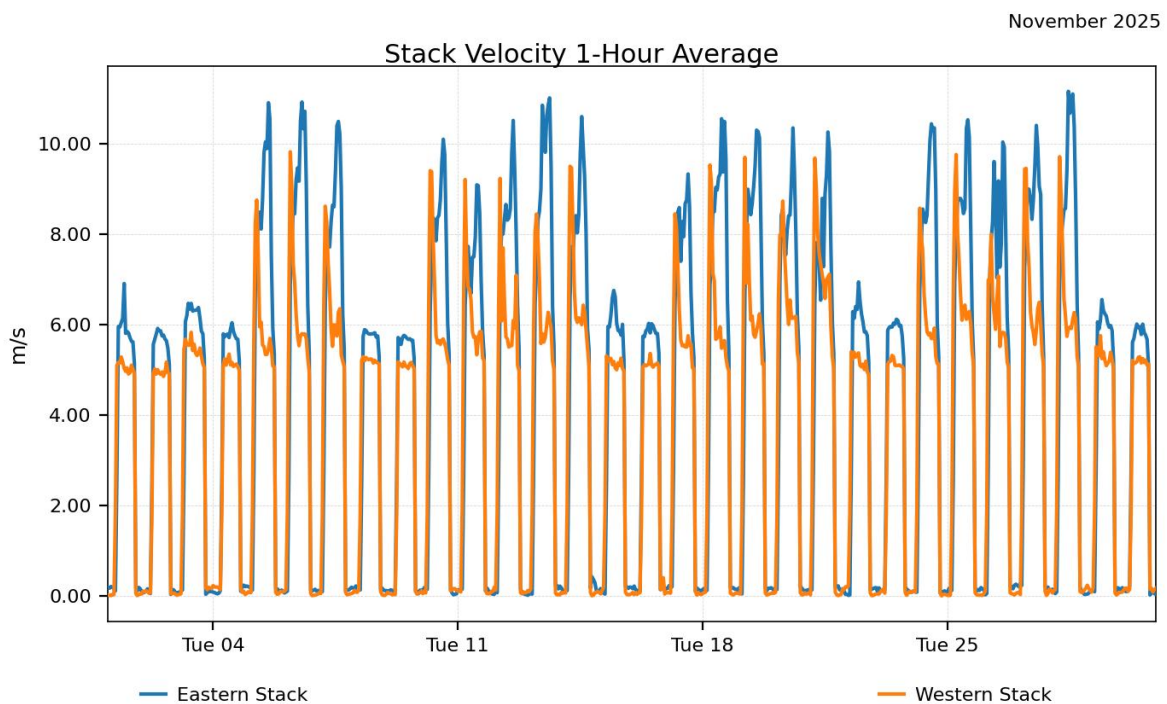


Figure 14. November 2025 Monthly 1-hour average stack velocity

7.4.3.7 November 2025 – Monthly 1-hour average stack temperature

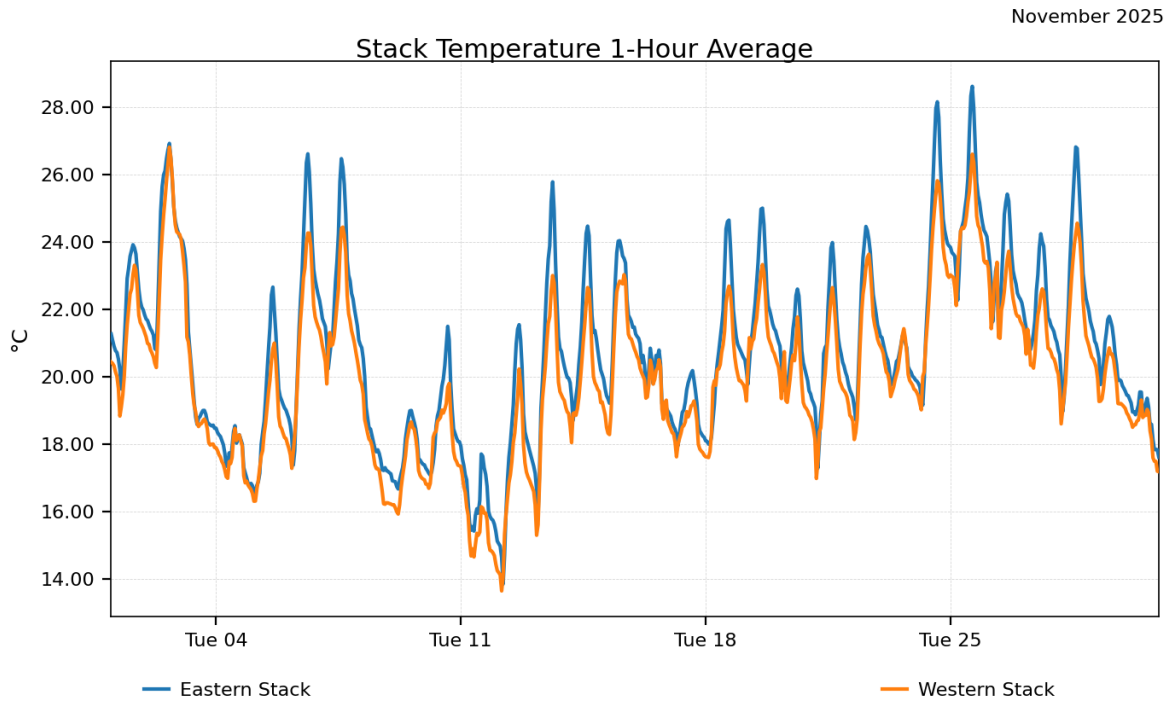


Figure 15. November 2025 Monthly 1-hour average stack temperature

7.4.4 December 2025

7.4.4.1 December 2025 – Monthly 1-hour mass rate NO₂

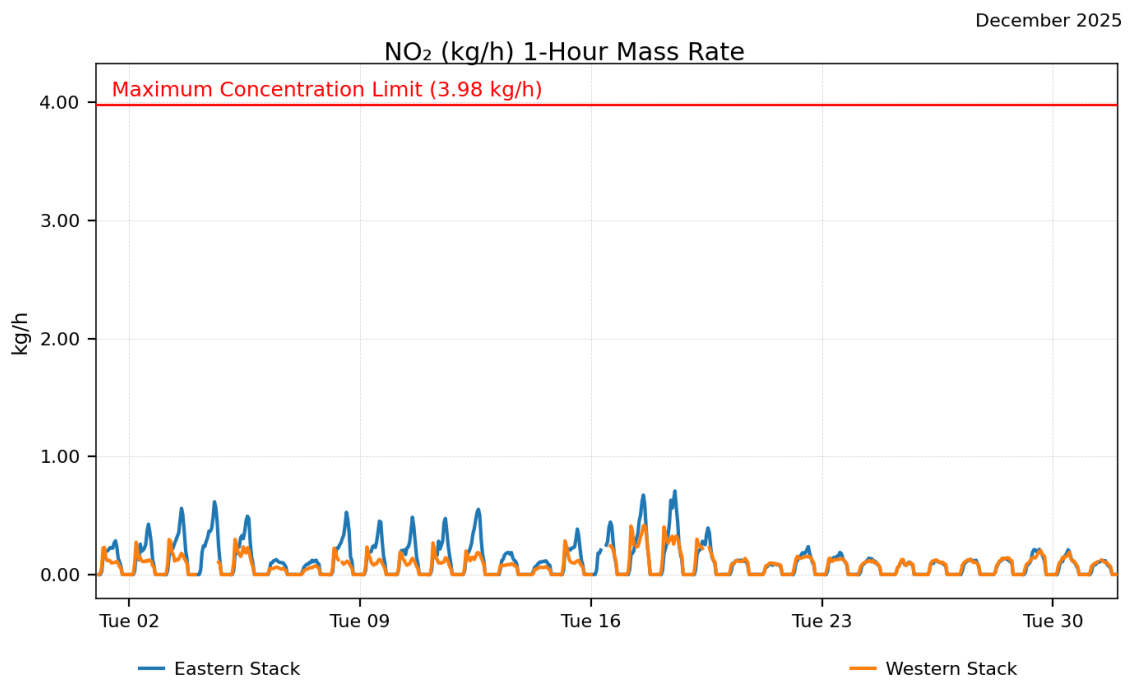


Figure 16. December 2025 Monthly 1-hour mass rate NO₂

7.4.4.2 December 2025 – Monthly 1-hour mass rate NO

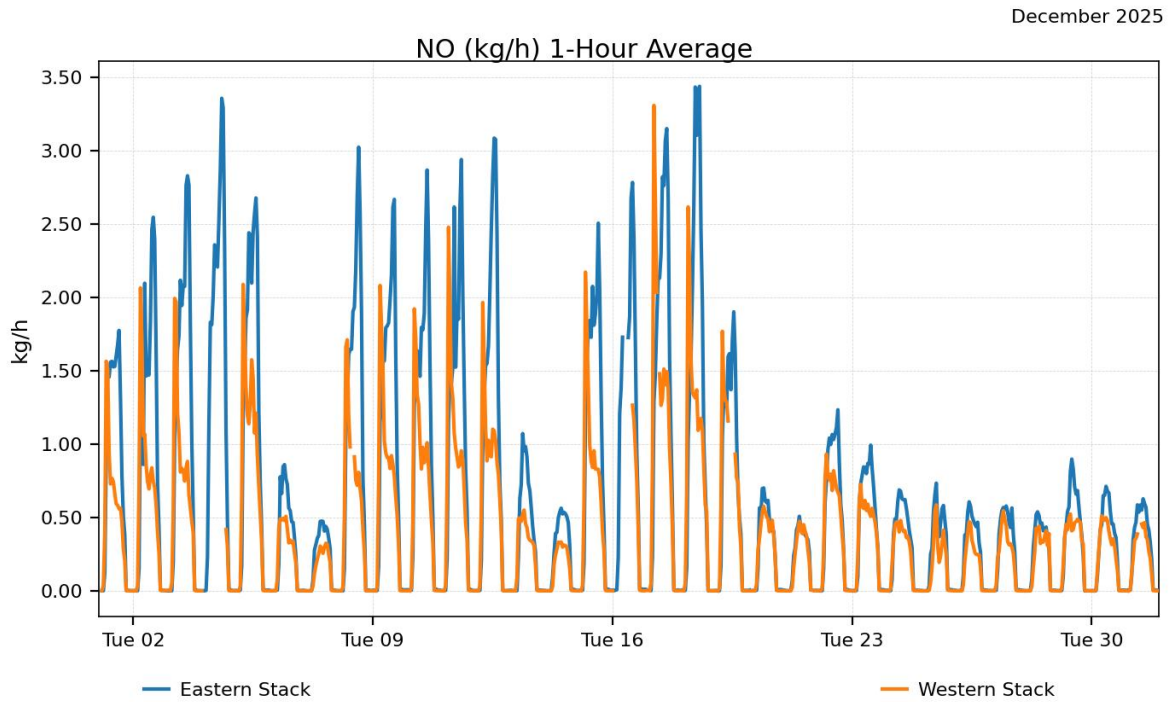


Figure 17. December 2025 Monthly 1-hour mass rate NO

7.4.4.3 December 2025 – Monthly 1-hour mass rate CO

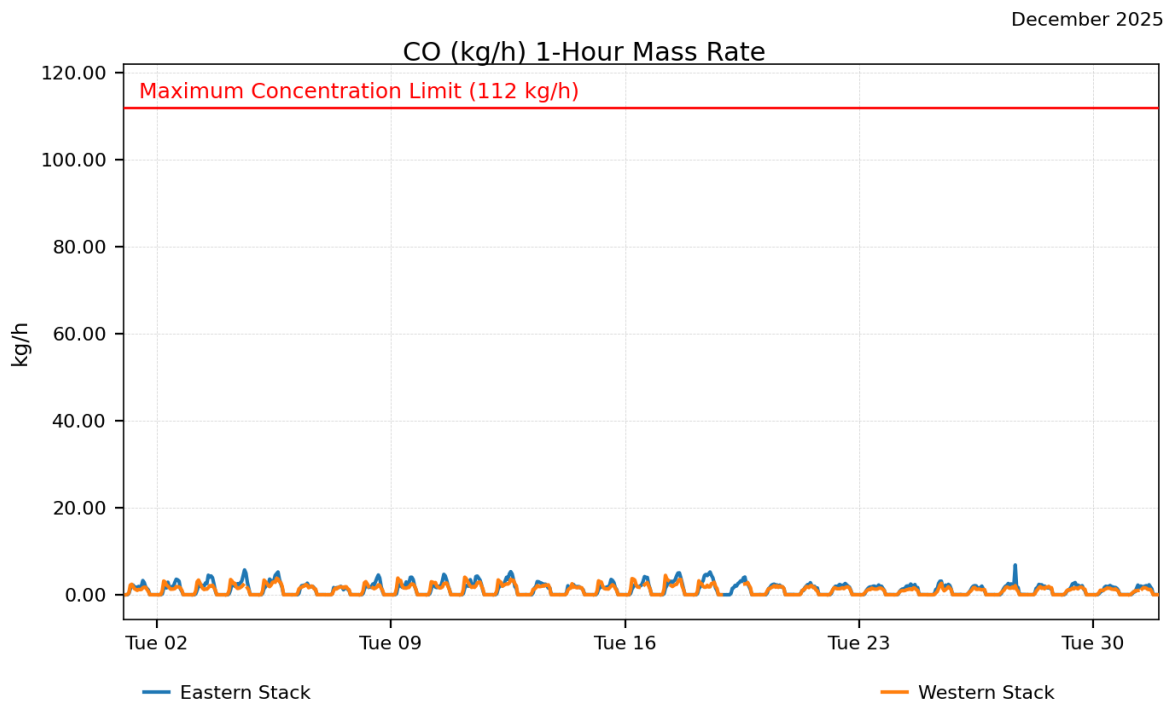


Figure 18. December 2025 Monthly 1-hour mass rate CO

8. Data Exceptions

This section outlines any issues noted with the monitoring equipment during the reporting period.

8.1 October 2025

8.1.1 October 2025 Western Ventilation Stack

EastLink Ventilation Western Ventilation Stack Data Validation – October 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/10/2025 0:00	7/10/2025 9:53	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 0.924146 Multiplier B: 0.924146	N/A	TA	19/01/2026
1/10/2025 23:45	31/10/2025 2:05	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
6/10/2025 1:46	8/10/2025 9:16	NO, NO ₂ , NO _x	Calibration out of tolerance	55.5	TA	19/01/2026
8/10/2025 9:17	8/10/2025 9:50	CO, NO, NO ₂ , NO _x	Maintenance	0.5	TA	19/01/2026
8/10/2025 9:51	21/10/2025 10:33	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.0 Multiplier B: 0.915742	N/A	TA	19/01/2026
21/10/2025 10:33	21/10/2025 11:28	CO, NO, NO ₂ , NO _x	Maintenance	0.9	TA	19/01/2026
29/10/2025 0:00	31/10/2025 23:59	CO	Offset applied to data: Offset A: -0.2 Offset B: -0.2	N/A	TA	19/01/2026

Table 24. October 2025 Western Ventilation Stack data validation

8.1.2 October 2025 Eastern Ventilation Stack

Eastlink Ventilation Eastern Ventilation Stack Data Validation - October 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/10/2025 0:00	8/10/2025 10:10	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.083378 Multiplier B: 1.083378	N/A	TA	19/01/2026
1/10/2025 0:00	30/10/2025 23:59	CO	Offset applied to data: Offset A: 0.1 Offset B: 0.1	N/A	TA	19/01/2026
1/10/2025 0:20	31/10/2025 10:33	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
8/10/2025 6:53	8/10/2025 6:54	All parameters	Missing data - data logger fault	0.0	TA	19/01/2026
8/10/2025 10:10	8/10/2025 10:35	CO, NO, NO ₂ , NO _x	Maintenance	0.4	TA	19/01/2026
11/10/2025 2:14	15/10/2025 1:34	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 0.933256 Multiplier B: 0.933256	N/A	TA	19/01/2026
12/10/2025 5:50	12/10/2025 10:18	PM _{2.5} , PM ₁₀	Unrealistic data - PM _{2.5} > PM ₁₀	4.5	TA	19/01/2026
14/10/2025 6:43	14/10/2025 6:43	All parameters	Missing data - data logger fault	0.0	TA	19/01/2026
21/10/2025 9:09	21/10/2025 10:13	CO, NO, NO ₂ , NO _x	Maintenance	1.1	TA	19/01/2026
30/10/2025 6:34	30/10/2025 6:35	All parameters	Missing data - data logger fault	0.0	TA	19/01/2026

Table 25. October 2025 Eastern Ventilation Stack data validation

8.2 November 2025

8.2.1 November 2025 Western Ventilation Stack

Eastlink Ventilation Western Ventilation Stack Data Validation - November 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/11/2025 0:00	30/11/2025 23:59	CO	Offset applied to data: Offset A: -0.2 Offset B: -0.2	N/A	TA	19/01/2026
1/11/2025 4:57	30/11/2025 23:40	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
19/11/2025 12:10	19/11/2025 12:44	PM _{2.5} , PM ₁₀	Unrealistic data - PM2.5 > PM10	0.6	TA	19/01/2026
22/11/2025 21:53	22/11/2025 23:41	PM _{2.5} , PM ₁₀	Unrealistic data - PM2.5 > PM10	1.8	TA	19/01/2026
23/11/2025 1:46	24/11/2025 10:26	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.087968 Multiplier B: 1.087968	N/A	TA	19/01/2026
24/11/2025 10:26	24/11/2025 11:14	CO, NO, NO ₂ , NO _x	Maintenance	0.8	TA	19/01/2026
26/11/2025 1:46	28/11/2025 11:22	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.104536 Multiplier B: 1.104536	N/A	TA	19/01/2026
28/11/2025 11:22	28/11/2025 12:00	CO, NO, NO ₂ , NO _x	Maintenance	0.6	TA	19/01/2026
28/11/2025 16:57	28/11/2025 17:24	CO, NO, NO ₂ , NO _x	Maintenance	0.4	TA	19/01/2026

Table 26. November 2025 Western Ventilation Stack data validation

8.2.2 November 2025 Eastern Ventilation Stack

Eastlink Ventilation Eastern Ventilation Stack Data Validation - November 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/11/2025 0:00	30/11/2025 23:59	CO	Offset applied to data: Offset A: 0.1 Offset B: 0.1	N/A	TA	19/01/2026
1/11/2025 0:49	30/11/2025 23:51	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
10/11/2025 7:00	10/11/2025 7:57	PM _{2.5} , PM ₁₀	Unrealistic data - PM2.5 > PM10	1.0	TA	19/01/2026
15/11/2025 2:14	24/11/2025 8:50	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.0 Multiplier B: 1.080481	N/A	TA	19/01/2026
18/11/2025 0:13	21/11/2025 4:31	CO	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
20/11/2025 0:28	20/11/2025 2:13	PM _{2.5}	Unrealistic data - PM2.5 > PM10	1.8	TA	19/01/2026
20/11/2025 6:27	20/11/2025 9:03	PM _{2.5}	Unrealistic data - PM2.5 > PM10	2.6	TA	19/01/2026
21/11/2025 4:43	21/11/2025 5:19	PM _{2.5}	Unrealistic data - PM2.5 > PM10	0.6	TA	19/01/2026
21/11/2025 9:23	21/11/2025 12:10	CO, NO, NO ₂ , NO _x	Maintenance	2.8	TA	19/01/2026
24/11/2025 8:50	24/11/2025 9:56	CO, NO, NO ₂ , NO _x	Maintenance	1.1	TA	19/01/2026

Table 27. November 2025 Eastern Ventilation Stack data validation

8.3 December 2025

8.3.1 December 2025 Western Ventilation Stack

EastLink Ventilation Western Ventilation Stack Data Validation – December 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/12/2025 0:00	16/12/2025 10:58	CO	Offset applied to data: Offset A: -0.2 Offset B: -0.2	N/A	TA	19/01/2026
1/12/2025 0:08	31/12/2025 10:58	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
4/12/2025 1:46	4/12/2025 15:36	NO, NO ₂ , NO _x	Calibration out of tolerance	13.8	TA	19/01/2026
4/12/2025 15:37	4/12/2025 17:13	CO, NO, NO ₂ , NO _x	Maintenance	1.6	TA	19/01/2026
5/12/2025 1:46	8/12/2025 9:24	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.062016 Multiplier B: 1.062016	N/A	TA	19/01/2026
8/12/2025 9:24	8/12/2025 10:50	CO, NO, NO ₂ , NO _x	Maintenance	1.4	TA	19/01/2026
9/12/2025 1:46	16/12/2025 1:00	NO, NO ₂ , NO _x	Multiplier applied to data: Multiplier A: 1.0 Multiplier B: 1.154277	N/A	TA	19/01/2026
16/12/2025 1:46	16/12/2025 10:57	NO, NO ₂ , NO _x	Calibration out of tolerance	9.2	TA	19/01/2026
16/12/2025 10:58	16/12/2025 13:18	CO, NO, NO ₂ , NO _x	Maintenance	2.3	TA	19/01/2026
17/12/2025 7:59	19/12/2025 0:04	CO	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
19/12/2025 0:17	19/12/2025 10:32	CO	Instrument fault	10.2	TA	19/01/2026
19/12/2025 10:33	19/12/2025 13:55	CO, NO, NO ₂ , NO _x	Maintenance	3.4	TA	19/01/2026
19/12/2025 13:57	31/12/2025 9:36	CO	Offset applied to data: Offset A: +0.6 Offset B: +1.6	N/A	TA	19/01/2026
31/12/2025 9:36	31/12/2025 10:53	CO, NO, NO ₂ , NO _x	Maintenance	1.3	TA	19/01/2026

Table 28. December 2025 Western Ventilation Stack data validation

8.3.2 December 2025 Eastern Ventilation Stack

Eastlink Ventilation Eastern Ventilation Stack Data Validation - December 2025						
Start Date	End Date	Parameters	Reason	Hours affected	User Name	Change Date
1/12/2025 0:00	31/12/2025 23:59	CO	Offset applied to data: Offset A: 0.1 Offset B: 0.1	N/A	TA	19/01/2026
1/12/2025 0:13	31/12/2025 0:45	PM _{2.5} , PM ₁₀	Intermittent unrealistic data - negative	N/A	TA	19/01/2026
16/12/2025 8:26	16/12/2025 10:33	CO, NO, NO ₂ , NO _x	Maintenance	2.1	TA	19/01/2026
16/12/2025 8:26	16/12/2025 12:41	PM _{2.5} , PM ₁₀	Maintenance	4.2	TA	19/01/2026
29/12/2025 5:04	29/12/2025 5:05	All parameters	Missing data - data logger fault	0.0	TA	19/01/2026

Table 29. December 2025 Eastern Ventilation Stack data validation

9. Report Summary

There were nil above-goal readings recorded during the reporting period.

10. Data validation explanations

Automatic background check refers to when analyser samples zero air and measures the level of the concentration voltage. This voltage is taken as the zero signal level and this value is subtracted from any subsequent readings as an active zero compensation. This is the analyser’s fine zero measurement.

Calibration check outside tolerance refers to when the calibration values are outside the tolerance limits set for the precision check.

Offset or Multiplier Applied to data refers to an offset or multiplier applied to the data. This operation may be performed for a number of reasons including: (a) when a clear trend / drift outside the tolerance limit can be demonstrated by repeated operation precision checks, (b) when a correction is required on previously logged data due to a calibration check being outside the allowable tolerance

Data transmission error refers to a period of time when the instrument could not transmit data. This may be due to a communication fault between the logger and the instrument.

Equipment malfunction/instrument fault refers to a period of time when the instrument was not in the normal operating mode and did not measure a representative value of the existing conditions.

Missing data/data not available refers to a period of time when either data has been lost or could not be collected.

Instrument Alarm refers to an alarm produced by the instrument. A range of alarms can be produced depending on how the operation of the instrument is being affected.

Instrument out of service refers to an unavailability of data due to an instrument being shut down for repair, maintenance, or factory calibration.

Logger error refers to when an error occurs and instrument readings are not correctly recorded by the logger.

Maintenance refers to a period of time when the logger / instrument was unavailable due to maintenance.

Overnight span/zero out of tolerance refers to when the span/zero reading measured by the analyser during an automatic precision check falls outside of the expected concentration limits.

Power Interruption refers to no power to the station therefore no data was collected at this time.

Remote Calibration refers to when a technician remotely connects to the station and manually performs a span check.

Warm up after power interruption refers to the startup period of an instrument after power has been restored.